RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

DrägerService®

Dräger

Gas Analyzer Tubing Replacement Guide

Part Number: SP00231
Rev: A
Date: 28 February 2002
© 2002 Draeger Medical, Inc.

Vitalert 3000

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

Vitalert 3000
Gas Analyzer Tubing Replacement Guide

This document is intended as a reference guide to assist in the replacement of gas analyzer assembly internal tubing. Item numbers in the following table are keyed to the numbers shown in the illustration on the next page.

Item	Description	Part Number	Kit Type	
			Maintenance 4117544-002	Contamination 4117544-001
1	Hose, Natural 0.075 ID	ML08003	X	X
2	Hose, Clear 0.130 ID	ML08007		X
3	Hose, Lined 1/16 ID	ML08017	X	X
4	Restrictor S18	4111758-003	X	X
5	Restrictor S34	4111758-004	X	X
6	T-fitting, 1/16 ID	4111437		X
7	Solenoid, 3-way	4111377		X
8	Fitting, 1/16 ID	4112707-001		X
9	L-fitting, 1/16 ID	4111756		X
10	L-fitting, 1/8 ID hose	4111770		X
11	L-fitting, 1/16 ID hose	4110173	X	X
12	Water Trap Reservoir	4110616	X	X
13	Sample Line, 6 Lg	4113334	X	X
14	Air Filter, Luer (M) x (F)	4111751	X	X
15	Sample Cell, 4610	S010194	X	X
16	Pump Assembly	4111764		X
17	Adjustable Restrictor	4107995		X
18	Hose Clamps	4110618-001		X

NOTE: Restrictors are stamped S18 and S34 for identification.

Gas Analyzer Tubing Replacement Guide (continued)

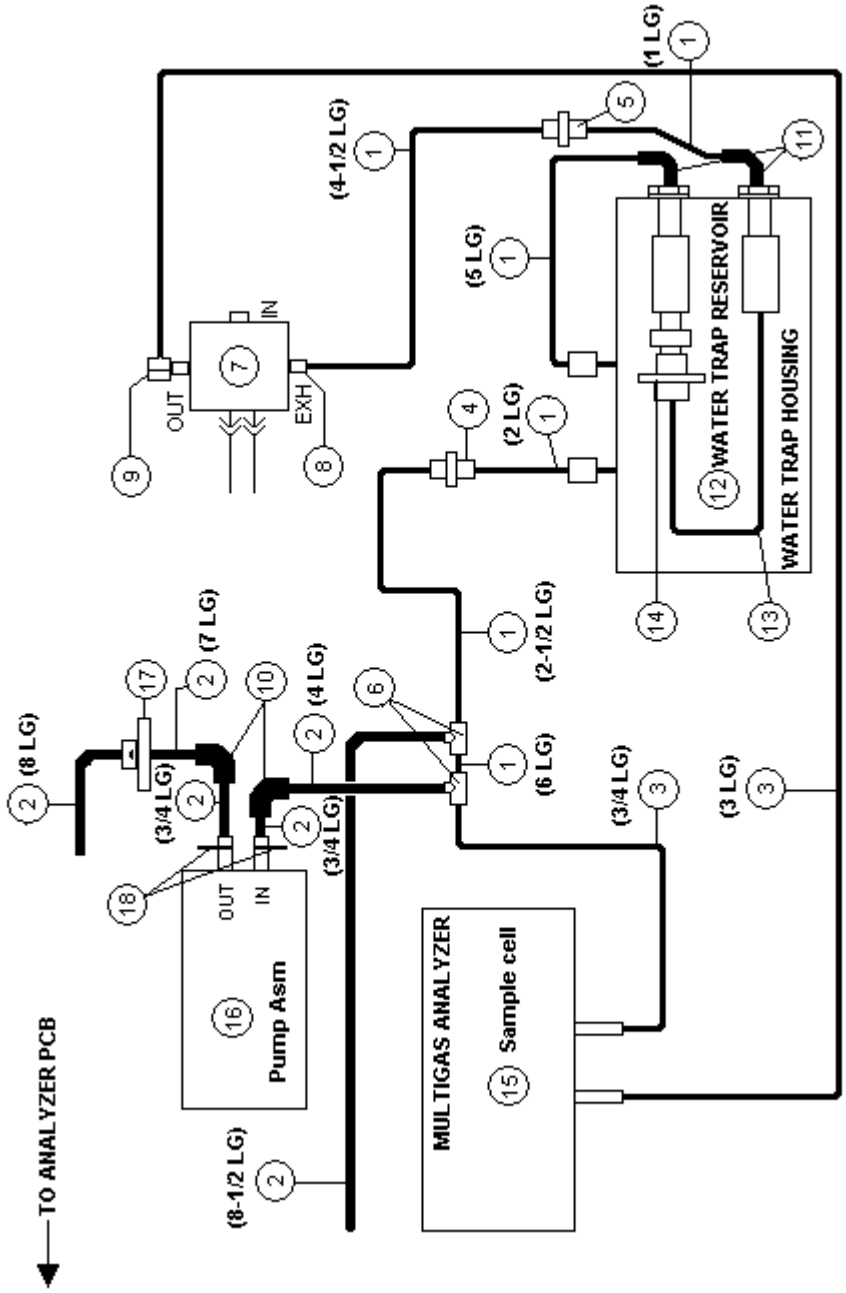

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

DrägerService®

Dräger

DrägerService is a division of
Draeger Medical, Inc.
3122 Commerce Drive
Telford, PA 18969
Tel: (215) 721-5402
(800) 543-5047
Fax: (215) 721-5784
Web: www.draegermedical.com
Printed in the U.S.A.